

Ralf Sussmann, Tobias Borsdorff, Markus Rettinger, and Frank Forster
IMK-IFU, Forschungszentrum Karlsruhe, Garmisch-Partenkirchen, Germany


One year of high-precision column measurements of CO₂ and CH₄ derived from near-infrared FTS at the TCCON site Garmisch (47.48 °N, 11.06 °E, 744m a.s.l.)

Abstract


Since 2007 at Garmisch, Germany (47.48 °N, 11.06 °E, 744m a.s.l.) a Bruker IFS125 HR near-infrared Fourier-Transform-Spectrometer is operated as part of the Total Carbon Column Observing Network (TCCON; <http://www.tccon.caltech.edu>). Solar absorption spectra in the wave number range 4000 - 16 000 cm⁻¹ are recorded continuously during clear sky conditions using dual acquisition from an InGaAs detector and a Si diode. From these spectra, accurate and precise column-averaged mixing ratios of CO₂ and CH₄ are retrieved using measured column ratios CO₂/O₂ and CH₄/O₂. These observations will be used to validate measurements of the NASA Orbiting Carbon Observatory (OCO) satellite mission and will also provide input data for the inverse modeling of sources and sinks of these Kyoto gases. Due to the high atmospheric background columns of CO₂ and CH₄ a single-column-measurement precision of better than 0.1% is required to be able to detect the relatively small effects from the sources and sinks of these species. This paper describes the observatory set up and shows an analysis of the first year of measurement data with a focus on quality control, and on annual as well as diurnal cycles of CO₂/O₂ and CH₄/O₂.

TCCON adaptations:


Detectors (Bruker D429/B) & (Bruker D510/B)

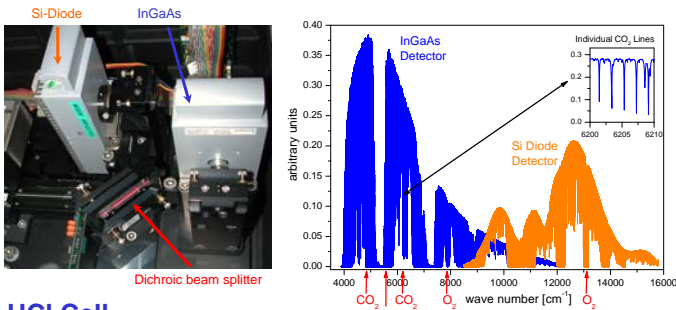

HCI Cell

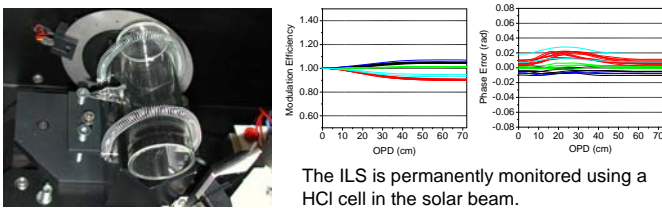


Pressure sensors

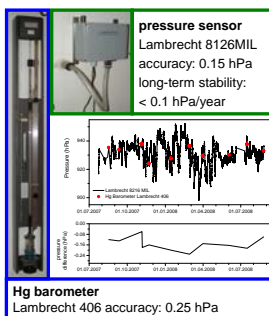

Solartracker



Time sync

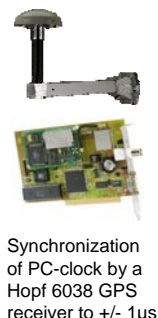


To achieve a single-column-measurement precision of better than 0.1% accurate solar tracking, surface pressure measurements and time synchronization are required.


GFIT retrieval results:

The nonlinear least squares profile scaling algorithm (GFIT) is used to retrieve CO₂, CH₄, O₂ column densities. The O₂ retrieval is used to convert the column densities to pressure-weighted column average mixing ratios.


Diurnal variation: cloudy day compared to clear sky day

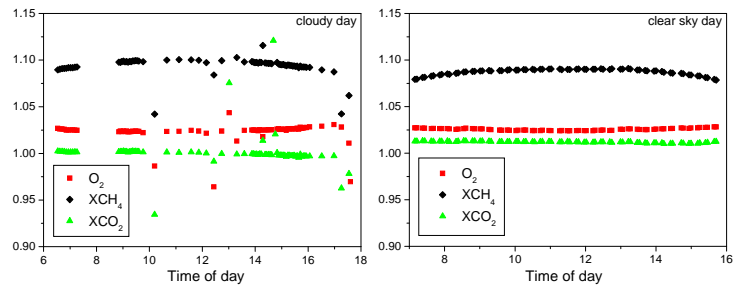

DC filtering: use InGaAs igrm instead of quadrant diode

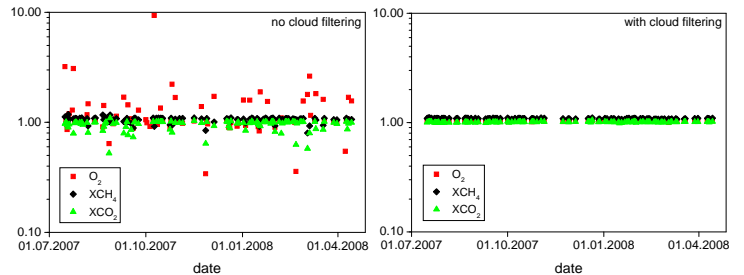

DC correction: implemented igrm-smoothing without fft

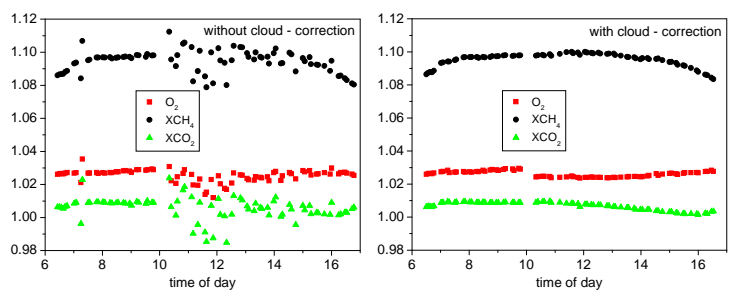

TCCON provides an essential validation resource:

The TCCON site Garmisch will provide ground-based validation and calibration for upcoming space-based instruments, such as the Orbiting Carbon Observatory (OCO) and Greenhouse Gases Observing Satellite (GOSAT).

